


THE COMPANY THAT PROFORMED THIS TEST REQUESTS CONFIDENTIALITY. THE FOLLOWING ARE REFLECTANCE MEASUREMENTS TAKEN WITH OUR ANALECT FTIR SPECTROMETER AT ZERO DEGREES (0°) ANGLE OF INCIDENCE AT ROOM AMBIENT TEMPERATURE (23°C).

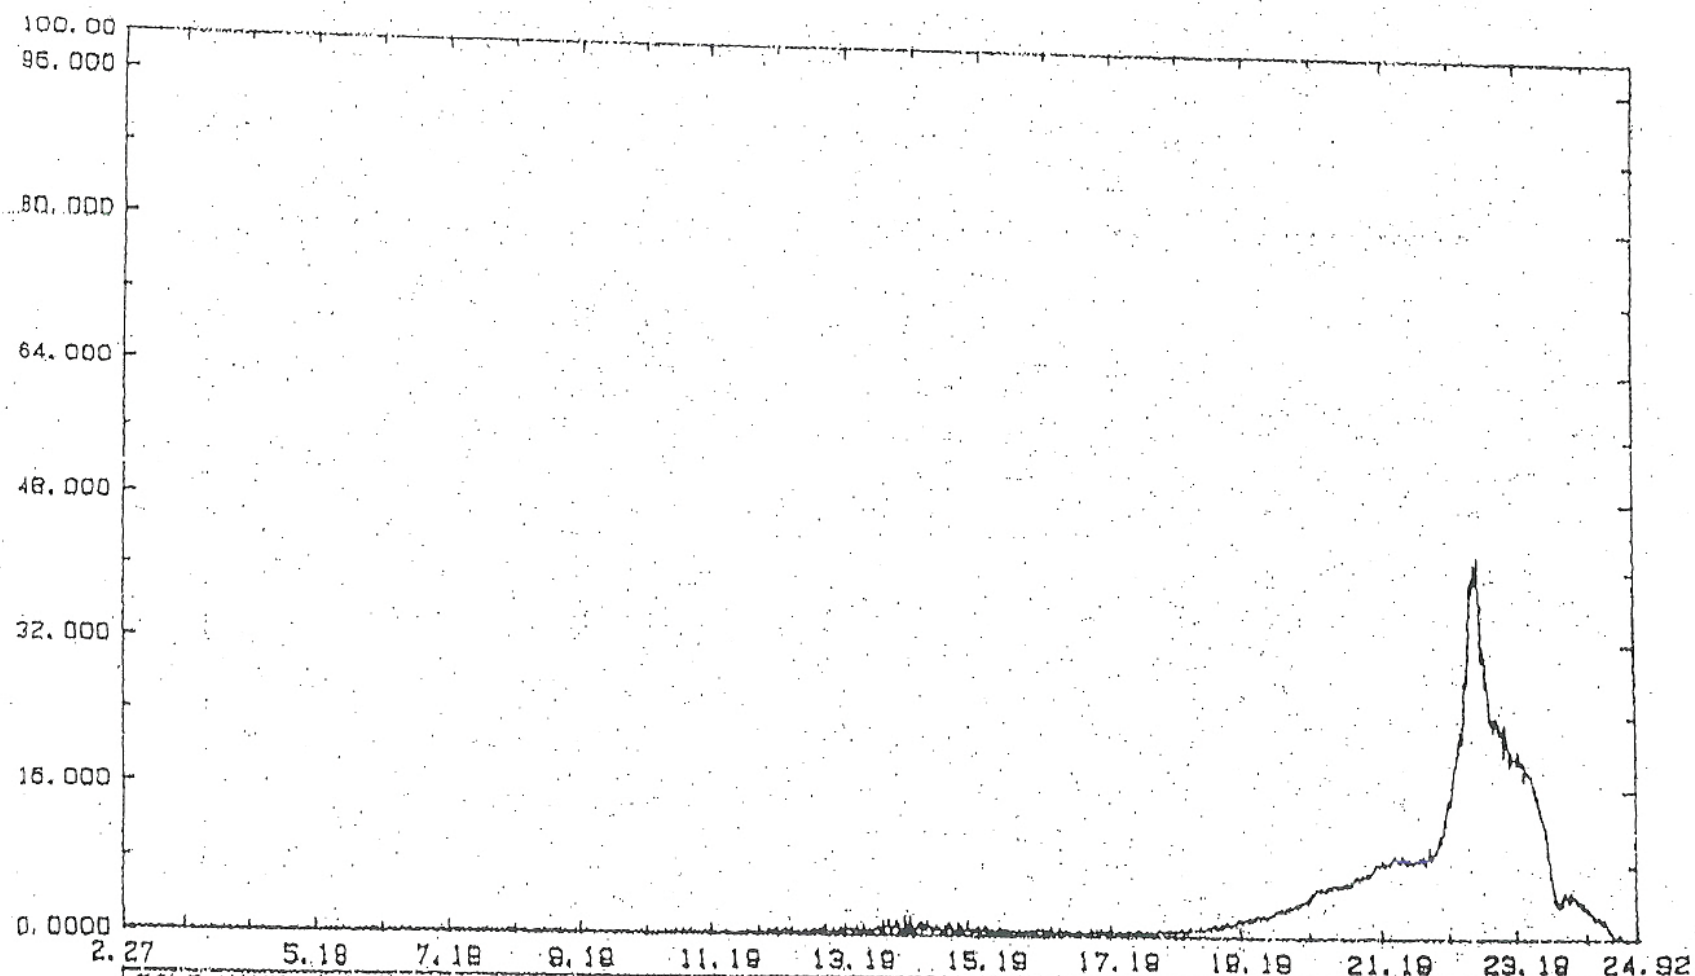

FILE NAME	: Sample #1	GAIN	: 128	ANALECT	AQS-20
#SCANS	: 32	DET	: TGS	ORD	: %T
#BKG	: 64	RES	: 4 CM-1	ABSC	: MICRON
APOD	: HAPP-GENZEL	DATE	: 12/12/17	TIME	: 04:36:47
COMMENT	: Epner Technology Filter w/ Black Coating				